



TPP SystmOne Integration

Please follow the instructions if you get labels printing without patient details.


Click on Setup > Mobile Working & Integration > Device Manager

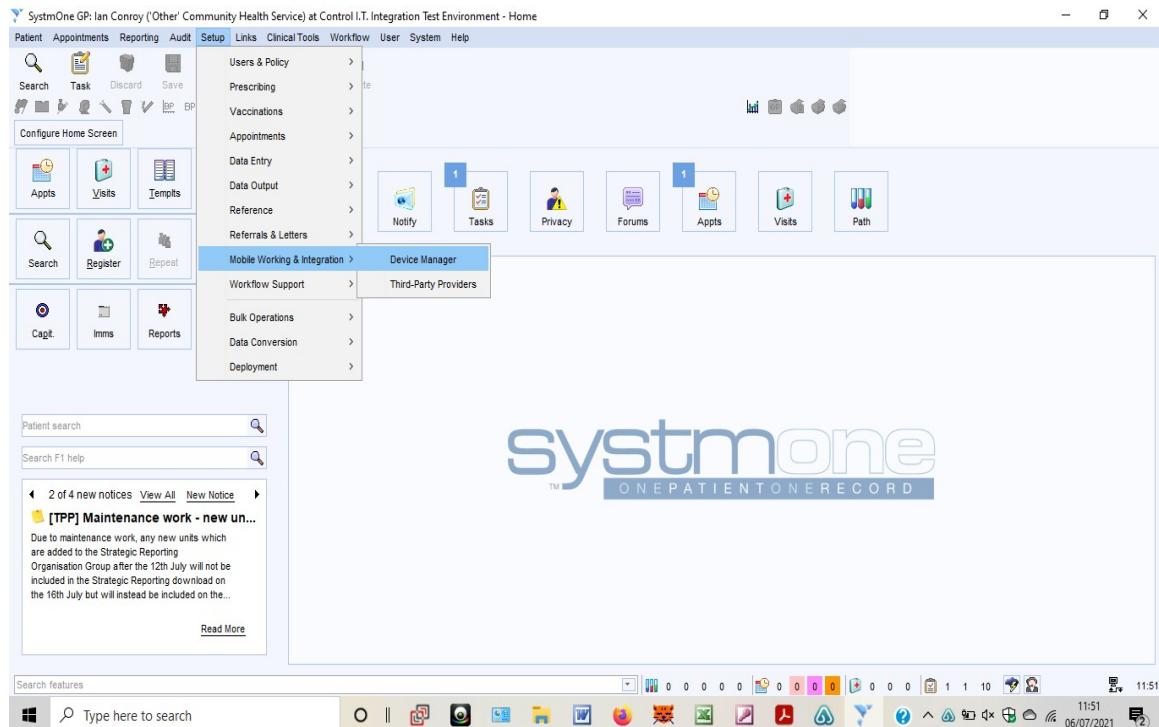

Double click on Blocked then right click on GPIT and select Approve Device. If more than one GPIT listed do the same on all of them.

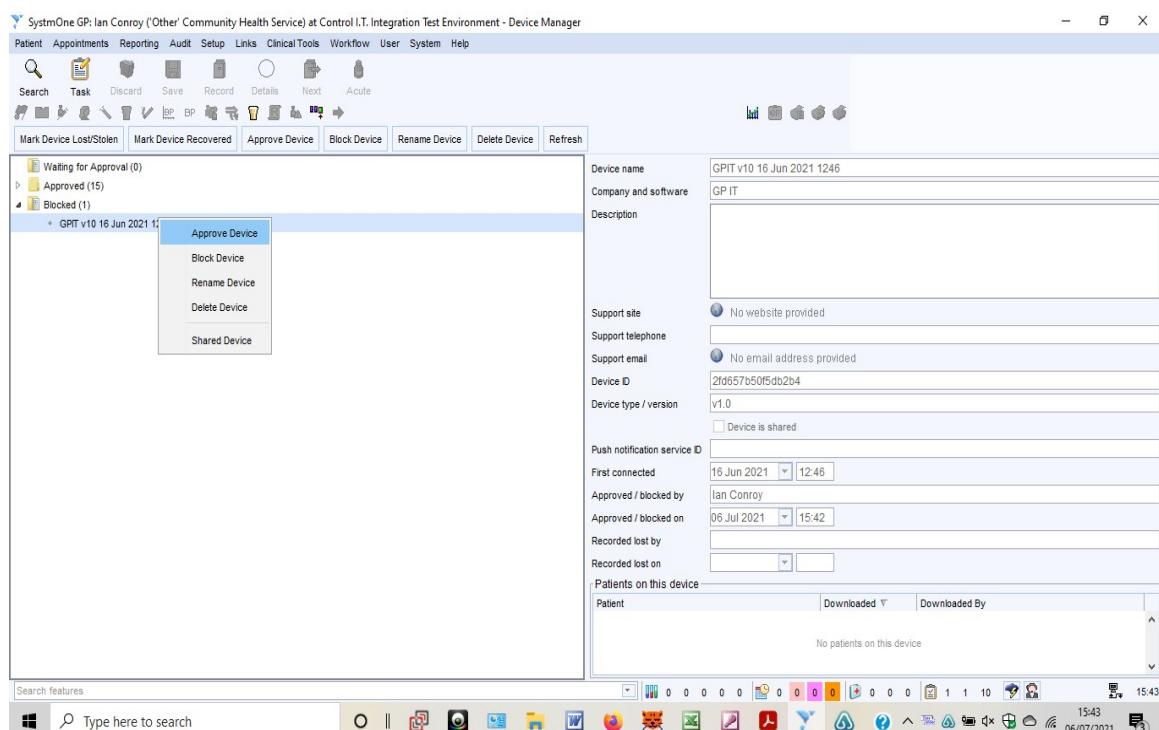

Click Yes on each one Approved

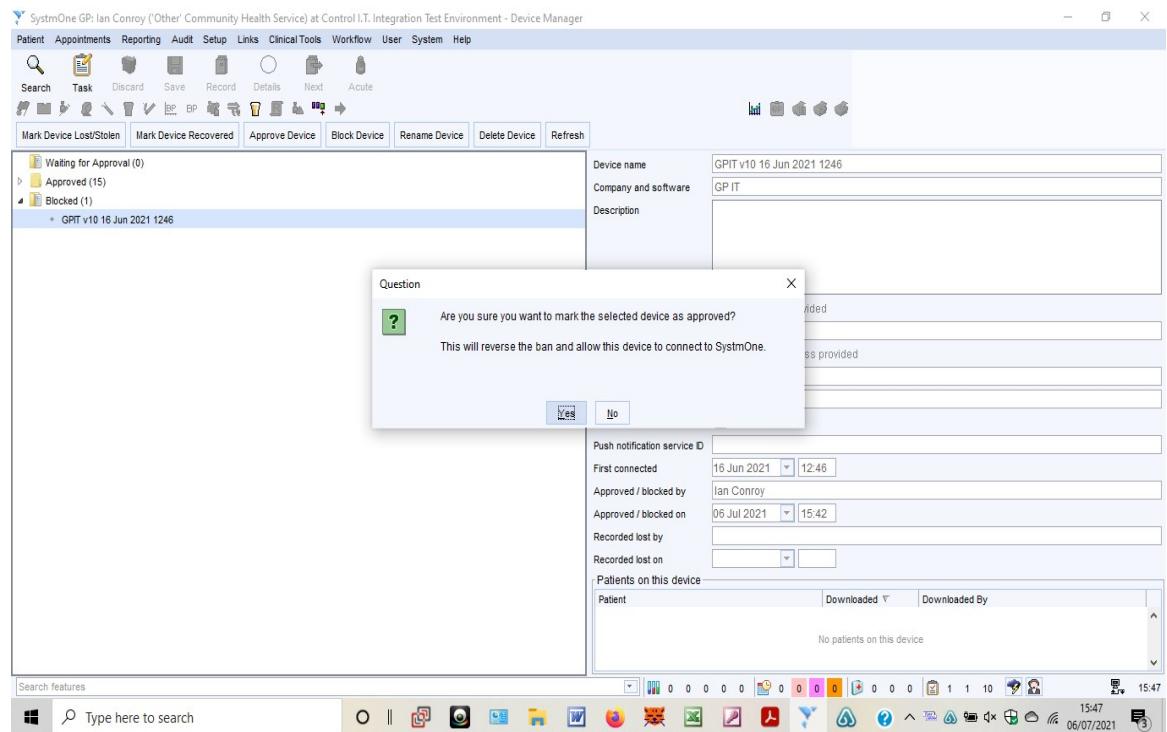

Once all have been Approved try printing a label